


Adductoplasty[®]

Midfoot Correction System




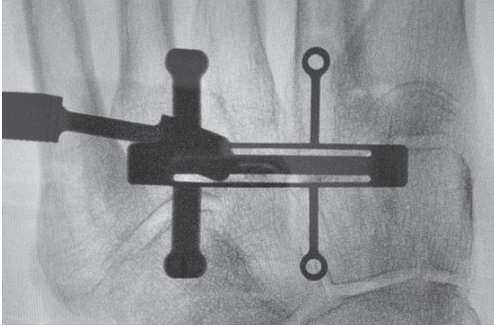
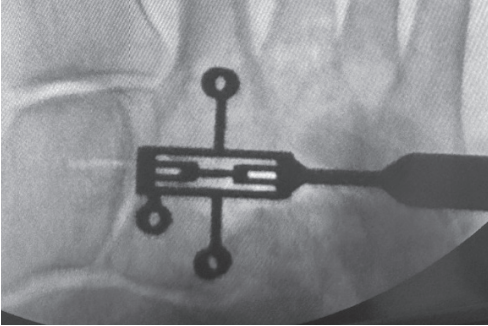


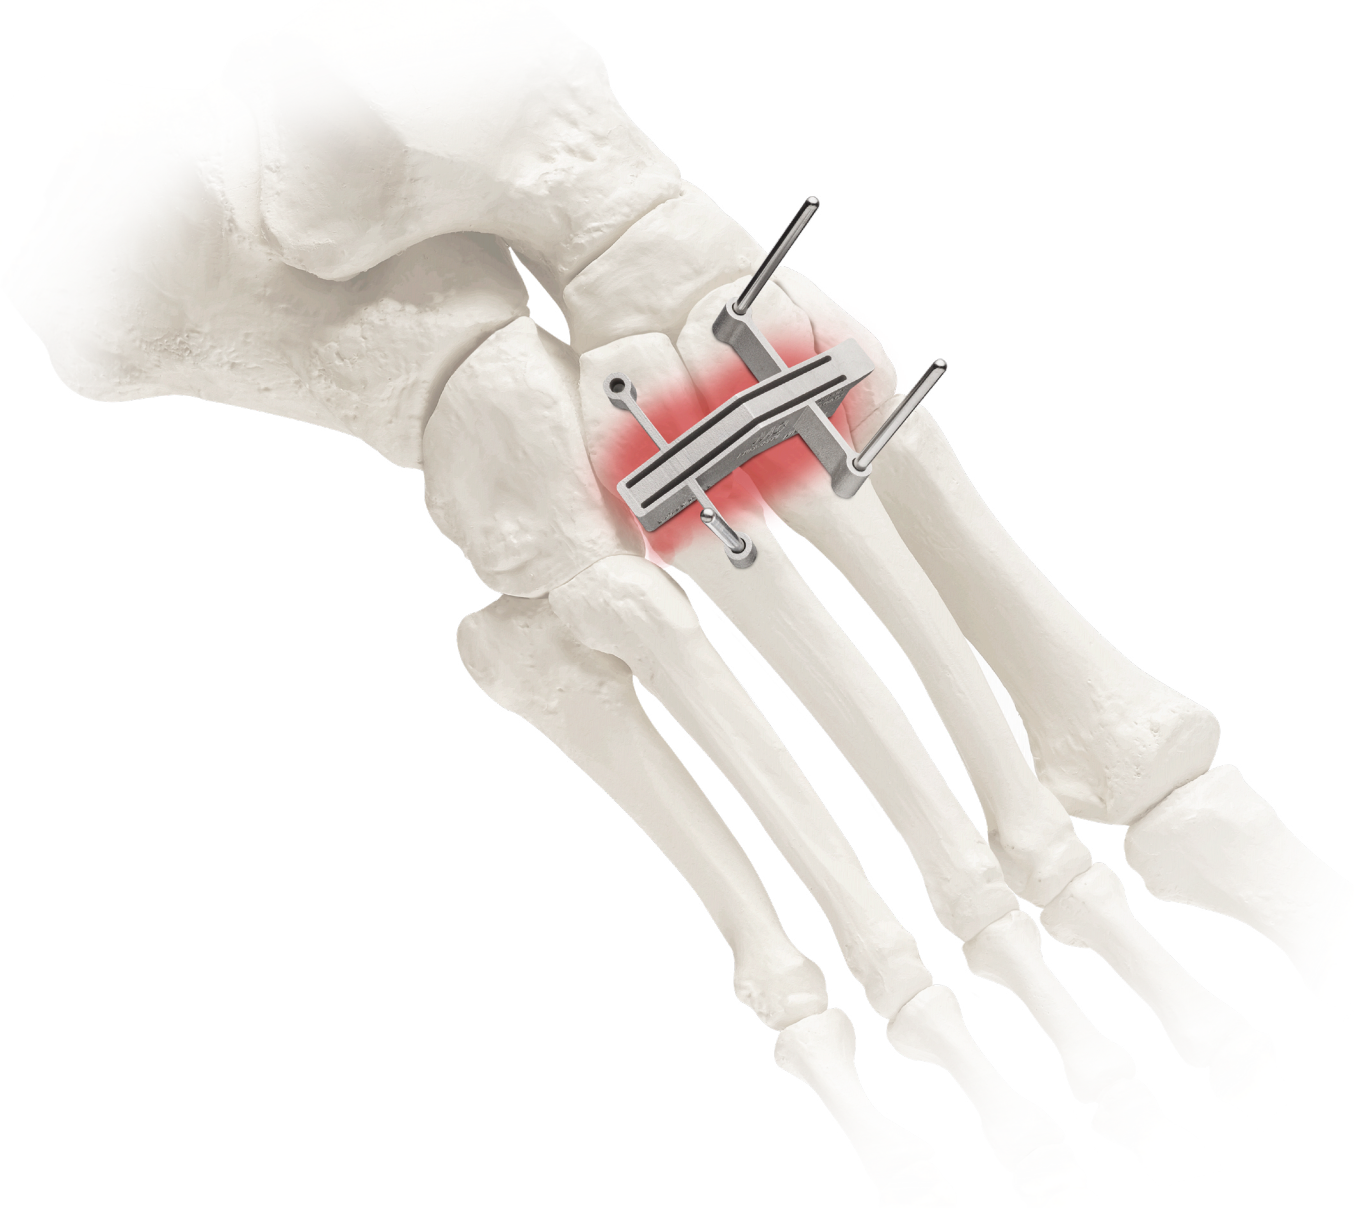




Precision Instrumentation Designed to Address Midfoot Arthritis

Adductoplasty[®]

Midfoot Correction System

Symptomatic midfoot OA is present in >10% of individuals 50+ years of age.¹ **Successful arthrodesis is associated with low nonunion rates, high levels of patient satisfaction, and improved AOFAS scores.^{2,3}** The Adductoplasty[®] System provides a comprehensive and reproducible solution for midfoot stabilization and fusion.

Key Surgical Steps	0° Cut Guide: Double Joint	0° Cut Guide: Single Joint
		
Plane		
		
Cut		
		
Compress		
		
Fixate		

Before use of the system, the surgeon should refer to the appropriate instructions for use and surgical technique for complete warnings, precautions, indications, contraindications, and adverse events. Risks include, but are not limited to: infection, pain, discomfort from the presence of the implant, loosening of the implant, and loss of correction with nonunion or malunion. If any of these occur, additional treatments may be needed. Additional information about risks, warnings, and instructions is available at Lapiplasty.com/surgeons/labeling.



To learn more, visit Lapiplasty.com



1 Thomas MJ, et al 2015. Arthritis Res Ther. 13;17(1):178. 2 Kurup H, et al. 2020.11(3):399-405. 3 Nemeč SA, et al. 2011 Foot Ankle Int. 11;32(4):355-361. Pat. treace.com/patents ©2024 Treace Medical Concepts, Inc. All rights reserved. M2524B