

FastGrafter[®]

Autograft Harvesting System



**Fully-sterile system for quick and efficient
harvest of autogenous bone**

FastGrafter®

Autograft Harvesting System

The FastGrafter® Autograft Harvesting System is a sterile-packed, single-use device designed for quick and efficient harvest of cancellous autogenous bone from the calcaneus, distal tibia, and other harvest sites through a minimal incision approach.


- **Single-piece** harvester designed to reduce instrumentation and system complexity
- **Morselizing cutting** tip penetrates cortex and morselizes bone during harvest
- **Sterile-packed system** designed for quick and efficient harvest of autograft bone

FastGrafter® Harvester



Calcaneal Autograft Harvest

Key surgical steps*

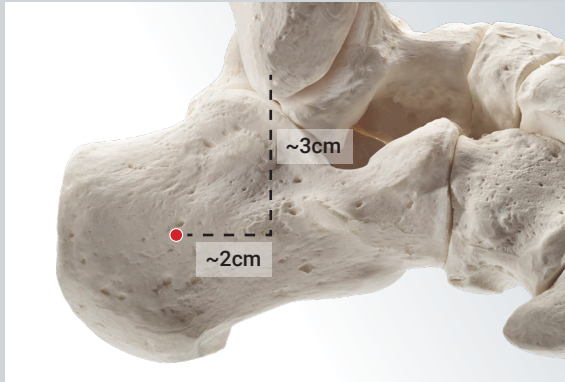

1.

Incision and Dissection

Make a small incision over the lateral aspect of the calcaneus, posterior and inferior to the peroneal tendon and sural nerve, approximately 3cm below and 2cm posterior to the distal fibula. Use blunt dissection to expose the bone.



2.

Bone Graft Harvest

Insert the **FastGrafter® Harvester** into AO attachment on a powered driver. Place the cutting tip of the **Harvester** onto the exposed bone surface. Beginning at low speed in the forward direction, advance the **Harvester** to the desired depth.



3.

Additional Bone Graft Harvest

Reinsert the **Harvester** tip into the original harvest site and make a pass approximately 20-30 degrees from the original harvest path.




4.

Removal of Morselized Bone Graft

Disassemble the **Harvester** from the powered driver. Over a sterile container, insert the **Pusher** through the distal tip of the **Harvester** to expel the morselized graft through the proximal opening of the **Harvester**.

Additional Harvest Sites

The FastGrafter® Autograft Harvesting System can be used percutaneously through multiple harvest sites including the calcaneus, proximal tibia, and distal tibia.

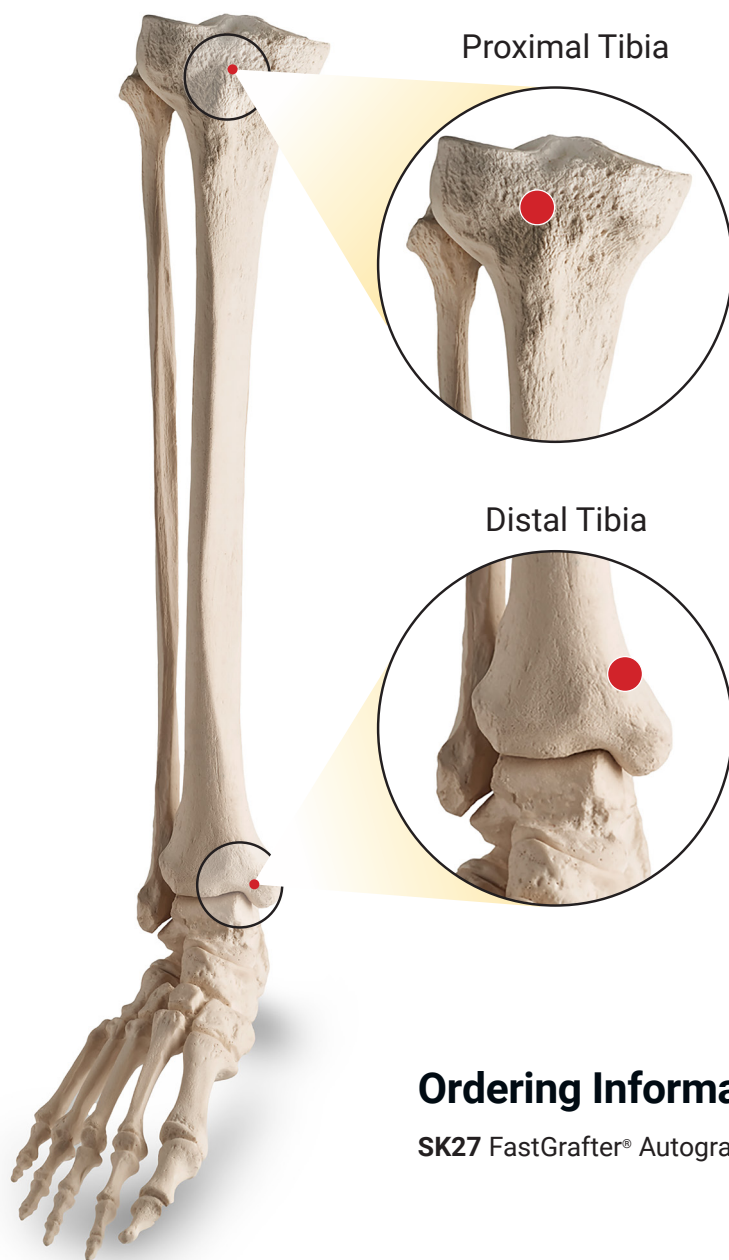

Ordering Information

SK27 FastGrafter® Autograft Harvesting System (7mm)

Before use of the instruments, the surgeon should refer to the appropriate instructions for use for complete warnings, precautions, indications, contraindications, and adverse events. Risks include, but are not limited to: infection, pain, discomfort, nerve or soft tissue damage, and necrosis of tissue or inadequate healing. If any of these occur, additional treatments may be needed. Additional information about risks, warnings, and instructions is available at Lapiplasty.com/surgeons/labeling.



To learn more, visit Lapiplasty.com

